

Application News

No. 078

Total Organic Carbon Analysis

Measurement of Total Carbon in Soil and Compost by TOC Solid Sample Measurement System



Soil contains a large amount of organic matter such as plant residue that can be decomposed by microorganisms. This organic matter plays a key role in plant growth by maintaining good chemical and physical conditions in soil and is useful in improving and stabilizing the productivity of agricultural crops. Compost, a type of fertilizer in which organic matter is decomposed by microorganisms, improves the condition of soil by supplying diverse substances and has the function of improving the growing condition of crops. Accordingly, determining the organic carbon content in soil provides a useful index for stable growth of agricultural crops and plants.

The Shimadzu TOC-L total organic carbon analyzer and SSM-5000A solid sample combustion unit comprise a system that enables measurement of the carbon content in solid samples. This article introduces an example of measurement of the total carbon content in soil and compost samples by using this Shimadzu TOC solid sample measurement system.

A. Goto

TOC Solid Sample Measurement System

The TOC solid sample measurement system (Fig. 1), consisting of a Shimadzu TOC-L total organic carbon analyzer and SSM-5000A solid sample combustion unit, quantifies the carbon content of a solid sample by combustion oxidation of the sample and detection of the formed carbon dioxide. Simple and quick analysis of the total carbon content is possible because extraction and other complicated, time-consuming pretreatment processes are not necessary.

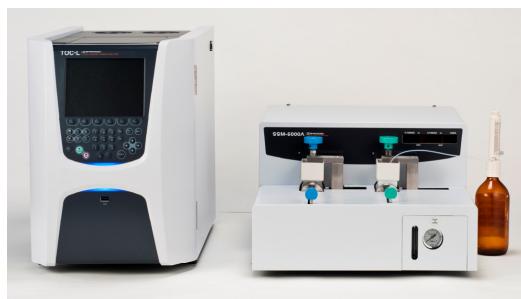


Fig. 1 TOC Solid Sample Measurement System

Analysis Method

In this experiment, two types of soil samples (soils A and B) and one type of compost sample were prepared. Fig. 2 shows the appearance of soil B. Approximately 100 mg of each sample was weighed in a sample boat (Fig. 3), and TC (total carbon) was measured. Table 1 shows the measurement conditions.



Fig. 2 Soil B Used in Measurement (Commercial Product)



Fig. 3 Weighing in Sample Boat

Table 1 Measurement Conditions

Analyzer	: TOC solid sample measurement system TOC-LCPH total organic carbon analyzer + SSM-5000A solid sample combustion unit
Cell length	: Short cell
SSM carrier gas	: Oxygen gas, 500 mL/min
TC oxidation method	: Catalytically aided combustion oxidation (TC oven temp.: 900 °C)
Measurement item	: TC (Total carbon)
Calibration curve	: One-point calibration curve using glucose powder reagent (Carbon concentration: 40%)
Samples	: Soil A: Collected from farm field Soil B: Commercial product Compost: Commercial product

■ Calibration Curve

A calibration curve for calibration of the analyzer was prepared by collecting and placing a glucose powder reagent (carbon concentration: 40%) in a sample boat and measuring its TC. Fig. 4 shows the measurement data.

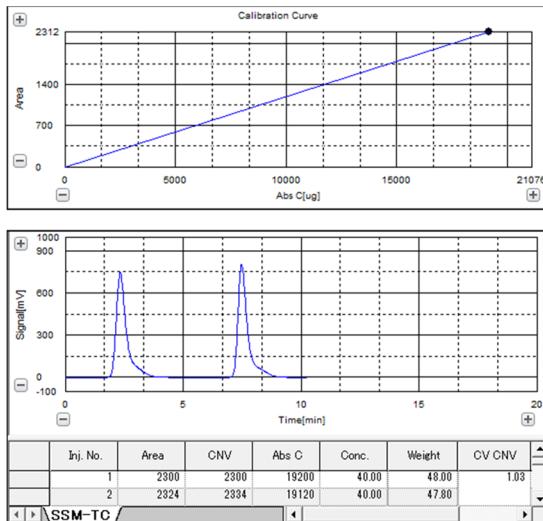


Fig. 4 Measurement Data for Calibration Curve

■ Sample Measurement Results

Fig. 5 shows the measurement data for the two soil samples (soils A and B) and the compost sample. Table 2 shows the measurement results for the three samples. Compost, being a fertilizer in which organic matter is decomposed by microorganisms, showed the highest TC concentration. It is thought that the commercial soil B displayed a higher TC concentration than soil A, which was collected from a farm field, because soil B is produced by blending fertilizer with the soil. Measurement with good repeatability was possible in all cases, as the coefficient of variation was 3% or less.

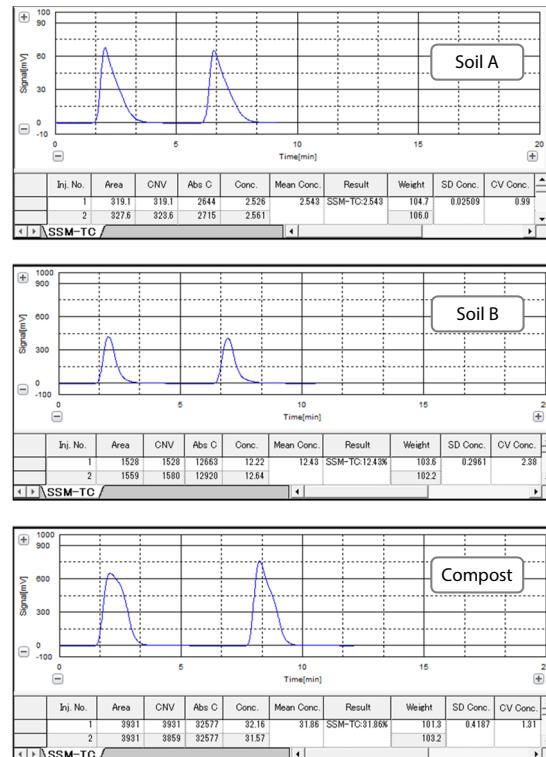


Fig. 5 Sample Measurement Data

Table 2 Measurement Results

Sample	TC concentration (%)	Coefficient of variation (%)
Soil A	2.543	0.99
Soil B	12.43	2.38
Compost	31.86	1.31

■ Conclusion

Use of the Shimadzu TOC solid sample measurement system made it possible to evaluate the differences in the total carbon content in soil and compost without extraction or other pretreatment procedures. Because simple and quick determination of the TOC in soil is possible, the system is expected to be useful in improving the productivity of agricultural products.

First Edition: Apr. 2020



Shimadzu Corporation

www.shimadzu.com/an/

For Research Use Only. Not for use in diagnostic procedure.

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

The content of this publication shall not be reproduced, altered or sold for any commercial purpose without the written approval of Shimadzu. Shimadzu disclaims any proprietary interest in trademarks and trade names used in this publication other than its own. See <http://www.shimadzu.com/about/trademarks/index.html> for details.

The information contained herein is provided to you "as is" without warranty of any kind including without limitation warranties as to its accuracy or completeness. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication. This publication is based upon the information available to Shimadzu on or before the date of publication, and subject to change without notice.

© Shimadzu Corporation, 2020